



CUSTOMER:	P/N: 0287.180	REV.	APPROVED BY:
-----------	---------------	------	--------------



REVISIONS		
REV.	DESCRIPTION	DATE
△		2011.03.07
△		2012/01/17
△		2012/04/19
△		2013/01/24
△		2014/02/20
△	Updates printing head	2014/12/05

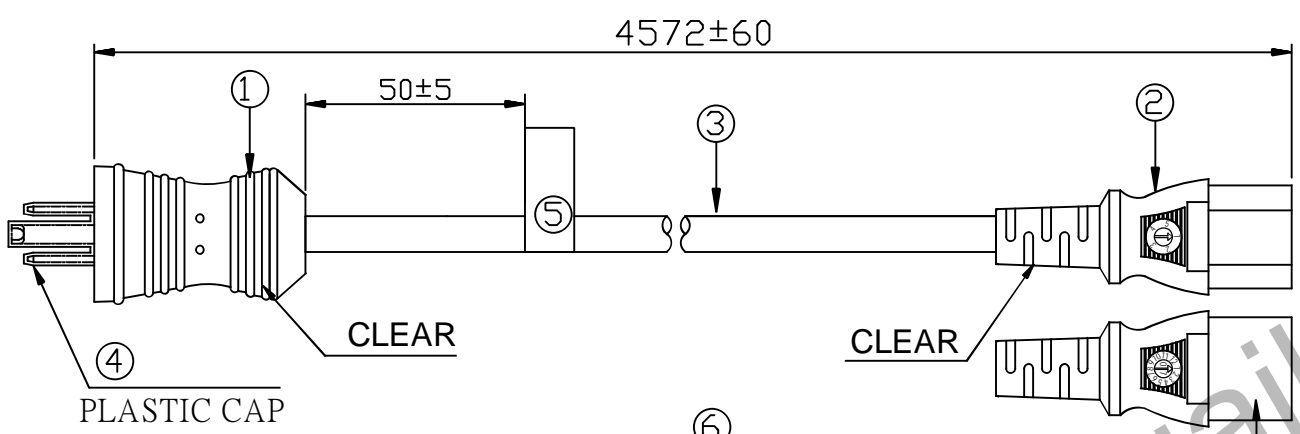

NOTES:
 1. CSA
 2. RoHS
 3. WS-002 tail transparent inner sleeve

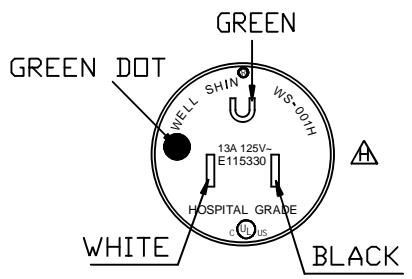


MARKING: CLEAR INSERT




⑤ Hosp.Grade label

NEMA 5-15P HOSPITAL GRADE CLEAR

IEC-60320-C13 CLEAR

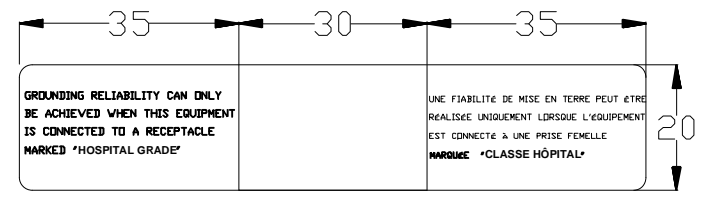

ITEM	DESCRIPTION	COLOR	Q'TY
⑥	Cable tie	BLACK	1
⑤	Hosp.Grade label	---	1
④	Plastic Cap	WHITE	1
③	SJT 16AWG*3C 105°C SHIELDED	BLACK	1
②	WS-002 13(A) 125(V)	CLEAR	1
①	WS-001H 13(A) 125(V)	CLEAR	1

ENGINEER BY:	SIGNATURE	 QUAIL ELECTRONICS, INC. http://www.quail.com	
MANAGER BY:			
CHECKED BY:		PRODUCT NO: 001H+002-1	DATE: 2014/12/05
DRAWN BY:		UNIT: mm	SHEET: 1 OF 1
		DWG NO: 0096-2058	REV. H